


THIS DRAWING AND SPECIFICATIONS ARE THE PROPERTY OF MICROSTRAIN INC. AND SHALL NOT BE REPRODUCED WITHOUT PERMISSION FROM MICROSTRAIN INC.

REVISIONS				1005-0007
ZONE	REV	DESCRIPTION	DATE	APPROVED
	A	ADD NOTE 1	9/10/03	SWM

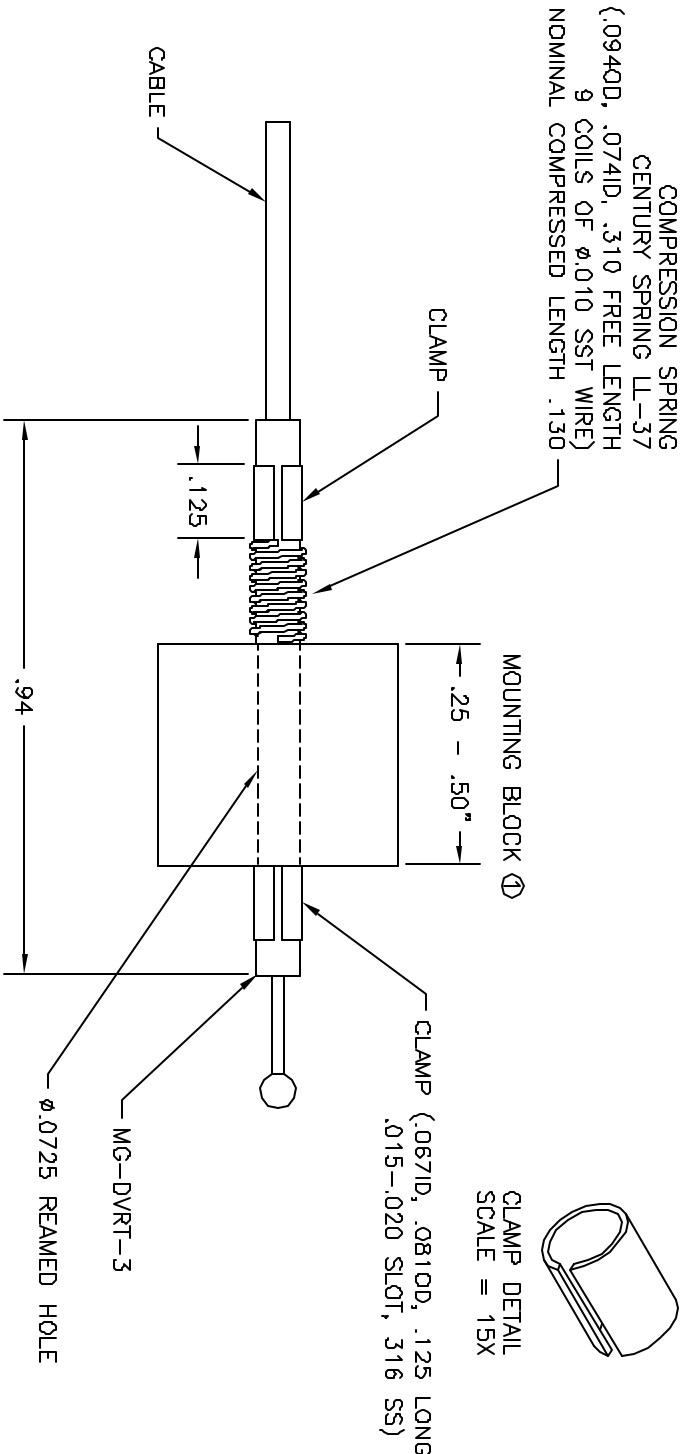

1. WE SUGGEST THAT THE MOUNTING BLOCK MATERIAL BE PLASTIC, 300 SERIES STAINLESS STEEL OR TITANIUM. MOUNTING IN MAGNETIC STEEL WILL REQUIRE RECALIBRATION. MOUNTING IN CONDUCTIVE MATERIAL (ALUMINUM, BRASS) WILL SIGNIFICANTLY REDUCE SENSOR OUTPUT AND REQUIRE RECALIBRATION.

UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES.  
TOLERANCES (UNOS)  
FRACTIONS:  $\pm 1/64$   
DECIMALS: .XX  $\pm .01$   
.XXX  $\pm .005$   
ANGLES:  $\pm 0.5$  DEGREES  
SURFACE FINISH: 63 MICROINCHES

**MicroStrain**  
310 Hurricane Lane, Suite 4  
Williston, VT 05495  
802-862-6629

**MG-DVRT-3 TYPICAL MOUNTING CONFIGURATION**

DRAWN BY: Stephen Pendo  
APPROVED BY:

SIZE: A  
CAGE CODE: 0XYZ9  
DWG NO.: 1005-0007  
REV: A

SCALE: 3:1  
DATE: 9 SEPT 2002  
SHEET: 1 OF 1